

Reference Material Certificate

112/02

Aluminium Base (Type of Standard)

Al pure (99.99-99.95% Al), Set 110

Certified Values

Element	Mass content [%]	Uncertainty [%]
Silicon (Si)	0.0009	± 0.0002
Iron (Fe)	0.0006	± 0.0001
Copper (Cu)	0.00020	± 0.00005
Manganese (Mn)	0.00002	± 0.00001
Magnesium (Mg)	0.00024	± 0.00005
Chromium (Cr)	0.00003	± 0.00002
Nickel (Ni)	<0.0001	
Zinc (Zn)	<0.0002	
Titanium (Ti)	0.00002	± 0.00001
Boron (B)	<0.0002	
Barium (Ba)	<0.00005	
Beryllium (Be)	<0.00002	
Bismuth (Bi)	0.00002	± 0.00001
Calcium (Ca)	<0.00003	
Cadmium (Cd)	<0.00002	
Cerium (Ce)	(<0.0001)	
Cobalt (Co)	<0.00002	
Gallium (Ga)	0.00003	± 0.00001
Lanthanum (La)	<0.00005	
Lithium (Li)	<0.00002	
Sodium (Na)	<0.00005	
Phosphorus (P)	0.0010	± 0.0002
Lead (Pb)	0.00010	± 0.00005
Antimony (Sb)	0.0003	± 0.0001
Tin (Sn)	<0.00002	
Strontium (Sr)	<0.00002	
Vanadium (V)	<0.0001	
Zirconium (Zr)	<0.0001	

The uncertainty reported is the result of standard deviation of all results multiplied with a factor of two and represents approximately the 95% confidence interval.

Values in brackets () are not certified but given for information only.

Manufacturing

This standard is produced using six strand hot top vertical continuous casting out of single melt.

Homogeneity

Homogeneity testing is performed by means of spark emission spectroscopy. Tests involve making multiple measurements on individual samples taken at regular intervals along the entire length of each cast rod. Depending on the mass content of the element, the relative standard deviation of multiple measurements between discs or within one disc is typically found between 0.3% - 1% for alloying and other elements and 0.5% - 5% for trace elements.

Analysis

The values listed in this analysis certificate are the results of multiple analyses performed in our chemical analysis laboratory which is an accredited test facility for aluminium alloys according to the international standard ISO 17025. The analyses are based on established wet chemical procedures.

Description of Sample


This reference material is available in the form of discs.

Intended use and Stability

This certified reference material is primarily intended for use in spark optical emission spectroscopy. Other applications are X-ray fluorescence spectrometry (XRF) and classical wet chemical procedures. The minimum sample size for wet chemical analysis is 0.2g. The material will remain stable for the period given below (certification validity) if it is stored in a dry and clean environment at room temperature.

Instructions for Use

Calibration measurements should be made within a ring between 2mm and 22mm from the edge of the CRM face. For wet chemical analysis chips have to be prepared by turning or milling of the sample surface.

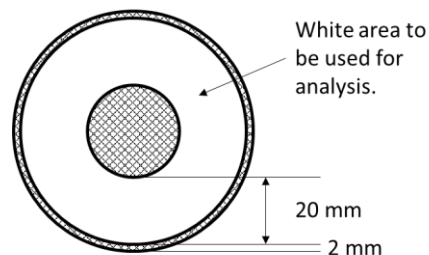

Traceability

Traceability of the certified mass contents to the SI (Système International d'Unités) is ensured by calibration using certified standard solutions or pure metals or substances of known stoichiometry.



Dr. Benedikt Moser
CTO



Patrik Bachmann
Head of Inorganic Analytics

Suisse Technology Partners Ltd.
Querstrasse 5
8212 Neuhausen am Rheinfall
Switzerland

Phone: +41 52 551 11 00
Fax : +41 52 551 11 99
Email: refmat@suisse-tp.ch
Internet: <https://reference-materials.ch>

Date of certification: 3-Jul-1995
Certificate version 003: 04-Jan-2022
This certificate is valid until: Jul-2070